

PTX 20 SUBMERSIBLE PRESSURE TRANSMITTERS (INSTALLATION GUIDE)



Status Business Park, Gannaway Lane
Tewkesbury, Glos. GL20 8FD. UK
Tel: +44 (0)1684 296818 Fax: +44 (0)1684 293746
Email: support@status.co.uk

Every effort has been taken to ensure the accuracy of this specification, however we do not accept responsibility for damage, injury, loss or expense resulting from errors and omissions, and we reserve the right of amendment without notice.

D2497-01-04



Important – Read this document before installing.

1.0 RECEIVING & UNPACKING

THIS PACKAGE CONTAINS DELICATE MEASUREMENT EQUIPMENT THAT REQUIRES CAREFUL HANDLING

Pressure transmitters are packed individually using suitable packing material which affords excellent protection for normal handling.

- 1) The external condition of the carton should be noted, with particular attention for signs of damage from impact or puncture.
- 2) When the goods are opened for inspection, ensure that the Operating Instructions and Calibration Certificate (if requested) are not accidentally lost or destroyed.
- 3) If the product has been specified for service with a critical media requiring special cleaning, the outer protection should not be removed unless under conditions of controlled cleanliness.
- 4) Do not touch, blow down or press against the measurement diaphragm as this can cause irreparable damage.

2.0 INSTALLATION

The installation should be undertaken in accordance with BS6739 - British Standard Code of practice for "Instrumentation in Process Control Systems: Installation Design and Practice."

All PTX transmitters are designed to withstand conditions normally found in process applications, however for maximum life and ease of maintenance the following guidelines should be observed.

- 1) Prior to installation, ensure the pressure source is not under pressure.
- 2) Avoid installing the pressure sensor in close proximity to motors, pumps, valves and heat sources. Excessive vibration or pressure peaks may falsify the sensor readings or even damage the sensor.
- 3) Use screened vented cable (if required) with the screen connected to earth at one end only.
- 4) Maximum supply voltage should not exceed 33 VDC

3.0 CALIBRATION

The unit can not be calibrated outside of the Factory – Please return for Re-Calibration.

4.0 WIRING


Colour	2-wire	3-wire
White	+Vin	+Vin
Yellow	Pout	GND
Brown		Pout
Grey	EP (only Ex)	

Supply Voltage (9 to 33) V DC
Atex Version (9 to 30) V DC

Load Resistance $RI = \frac{(V_{supply} - 9)}{0.02 A}$

5.0 MECHANICAL

Closed Version

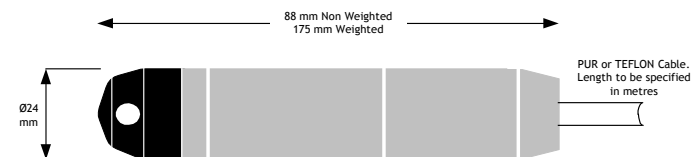

Open Version

